The
Patent
Office

INVESTOR IN PEOPLE

The Patent Office
Concept House
Cardiff Road
Newport
South Wales
NP10 8Q REC'D **1 3 JUL 2004**

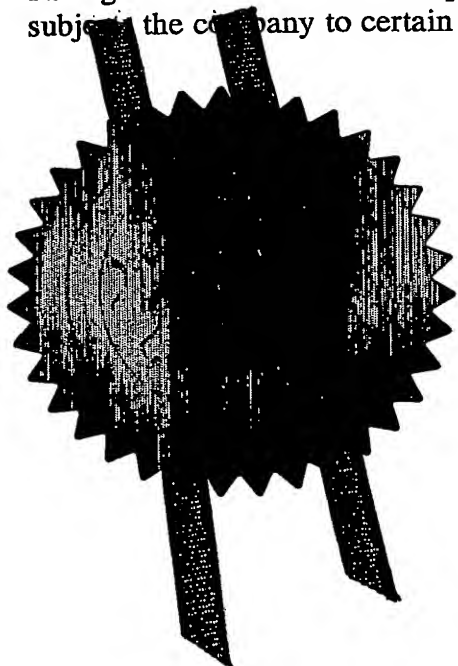WIPO   PCT

PRIORITY DOCUMENT

SUBMITTED OR TRANSMITTED IN
COMPLIANCE WITH RULE 17.1(a) OR (b)

I, the undersigned, being an officer duly authorised in accordance with Section 74(1) and (4) of the Deregulation & Contracting Out Act 1994, to sign and issue certificates on behalf of the Comptroller-General, hereby certify that annexed hereto is a true copy of the documents as originally filed in connection with the patent application identified therein.

In accordance with the Patents (Companies Re-registration) Rules 1982, if a company named in this certificate and any accompanying documents has re-registered under the Companies Act 1980 with the same name as that with which it was registered immediately before re-registration save for the substitution as, or inclusion as, the last part of the name of the words "public limited company" or their equivalents in Welsh, references to the name of the company in this certificate and any accompanying documents shall be treated as references to the name with which it is so re-registered.

In accordance with the rules, the words "public limited company" may be replaced by p.l.c., plc, P.L.C. or PLC.

Re-registration under the Companies Act does not constitute a new legal entity but merely subjects the company to certain additional company law rules.

Signed

Dated   7 June 2004

Patents Form 1/77

Act 1977
(Rule 16)

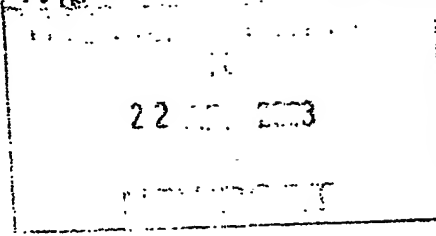The Patent Office
Patents • Designs • Copyright • Trade Marks

19APR03 E801361-3 D02884
P01/7700 0.00-0309025.5

1/77

Request for grant of a patent

(See the notes on the back of this form. You can also get an explanatory leaflet from the Patent Office to help you fill in this form)

22 ... 2003

The Patent Office

Cardiff Road
Newport
South Wales
NP10 8QQ

1.	Your reference	P34031/GWO/JCO

2. **Patent application number**
(The Patent Office will fill in this part)

0309025.5

22 APR 2003

3. Full name, address and postcode of the or of each applicant *(underline all surnames)*

1) John Andrew Murray McGRATH, 4 Randolph Cliff, Edinburgh EH3 7TZ; and 2) John Scott STRACHAN, 6 Marchhall Crescent, Edinburgh EH16 5HN

Patents ADP number *(if you know it)*

1) 40779 54 001
2) 426 176 4003

If the applicant is a corporate body, give the country/state of its incorporation

4. Title of the invention

Method and Apparatus for the Early and Rapid diagnosis of Glaucoma and other Human and Higher Primate Visual Disorders

5. Name of your agent *(if you have one)*

Murgitroyd & Company

"Address for service" in the United Kingdom to which all correspondence should be sent *(including the postcode)*

Scotland House
165-169 Scotland Street
Glasgow
G5 8PL

Patents ADP number *(if you know it)*

1198015

6. If you are declaring priority from one or more earlier patent applications, give the country and the date of filing of the or of each of these earlier applications and *(if you know it)* the or each application number

Country	Priority application number *(if you know it)*	Date of filing *(day / month / year)*

7. If this application is divided or otherwise derived from an earlier UK application, give the number and the filing date of the earlier application

Number of earlier application	Date of filing *(day / month / year)*

8. Is a statement of inventorship and of right to grant of a patent required in support of this request? *(Answer 'Yes' if:*
a) *any applicant named in part 3 is not an inventor, or*
b) *there is an inventor who is not named as an applicant, or*
c) *any named applicant is a corporate body.*
See note (d))

No

Patents Form 1/77

Patents Form 1/77

9. Enter the number of sheets for any of the
following items you are filing with this form.
Do not count copies of the same document

Continuation sheets of this form

Description	17
Claim(s)	2
Abstract	-
Drawing(s)	-

10. If you are also filing any of the following,
state how many against each item.

Priority documents	-
Translations of priority documents	-
Statement of inventorship and right to grant of a patent *(Patents Form 7/77)*	-
Request for preliminary examination and search *(Patents Form 9/77)*	-
Request for substantive examination *(Patents Form 10/77)*	-
Any other documents *(please specify)*	-

11.

I/We request the grant of a patent on the basis of this application.

Signature *[signature]*

Murgitroyd & Company

Date
17 April 2003

12. Name and daytime telephone number of
person to contact in the United Kingdom

JOHN COOPER   0141 307 8400

Warning

After an application for a patent has been filed, the Comptroller of the Patent Office will consider whether publication or communication of the invention should be prohibited or restricted under Section 22 of the Patents Act 1977. You will be informed if it is necessary to prohibit or restrict your invention in this way. Furthermore, if you live in the United Kingdom, Section 23 of the Patents Act 1977 stops you from applying for a patent abroad without first getting written permission from the Patent Office unless an application has been filed at least 6 weeks beforehand in the United Kingdom for a patent for the same invention and either no direction prohibiting publication or communication has been given, or any such direction has been revoked.

Notes

a)   *If you need help to fill in this form or you have any questions, please contact the Patent Office on 08459 500505.*

b)   *Write your answers in capital letters using black ink or you may type them.*

c)   *If there is not enough space for all the relevant details on any part of this form, please continue on a separate sheet of paper and write "see continuation sheet" in the relevant part(s). Any continuation sheet should be attached to this form.*

d)   *If you have answered 'Yes' Patents Form 7/77 will need to be filed.*

e)   *Once you have filled in the form you must remember to sign and date it.*

f)   *For details of the fee and ways to pay please contact the Patent Office.*

"METHOD AND APPARATUS FOR THE EARLY AND RAPID DIAGNOSIS OF GLAUCOMA AND OTHER HUMAN AND HIGHER PRIMATE VISUAL DISORDERS"

BACKGROUND TO INVENTION

1
2 The common form of Glaucoma, as is typical of several other visual disorders, is a
3 progressive disease. Currently the disease can be arrested but not cured. Symptoms
4 include the gradual reduction in the field of view of the affected eye progressing in a
5 characteristic pattern. Due to the nature of the human visual system, victims of the
6 disease do not typically notice this reduction in field of view until the disease has already
7 progressed for several years. Instruments exist which can measure the field of view of a
8 patient but all available instruments suffer from three major problems that limit their
9 utility in making an early diagnosis. First they are both low in resolution and inaccurate.
10 This low resolution means that the slow progression of the disease at typically 1.8% of
11 the field of view per annum can take several years to be detectable.
12 "Relative rates of disc and field change examined in eyes at high risk"
13 C Scerra Ophthalmology times 15/10/2001
14 Secondly the existing devices and methods are slow and complex in clinical use and
15 hence expensive in practitioner time. This means that even those practitioners who
16 possess a field of view analysis device cannot economically use it as a routine screening
17 device. Thirdly the existing instruments are inherently expensive and so are not as
18 widely available as is required for the widespread screening necessary for early diagnosis.
19 At one time it was thought that measurement of eyeball pressure would provide a
20 method for early diagnosis of glaucoma but this has proved unreliable as the correlation
21 between pressure and glaucoma has proved not to be as high as was originally thought.
22 Instruments for the measurement and mapping of the sensitivity of the human retina
23 known as "visual field analyzers" or "Static Auto-perimeters" have hitherto required
24 that the subject perform very unnatural and often uncomfortable eye behaviors such as
25 long periods of attempted fixation on a point. Additionally, hitherto such instruments
26 depended on tests requiring a voluntary response from the subject. The subject is asked
27 to concentrate on a fixation point and report on the presence and position of stimuli
28 presented to their peripheral vision. This process is both slow and prone to inaccuracy.
29 The ability of the subject to accurately fixate is also known to be poor especially over an
30 extended period and so the accuracy of a purely fixation point to stimulus measurement
31 is further compromised.
32 This invention substantially reduces or eliminates these problems and introduces an
33 entirely novel method and apparatus that allows the subject under test to behave
34 completely naturally (in the sense that they are not required to suppress natural visual
35 reflexes) which both improves accuracy and lowers the stress on the subject.
36 Furthermore the disclosed method and apparatus greatly reduces the time required to
37 map the visual field, which makes the test far more economic and practical for routine
38 screening than the existing equipment that requires lengthy tests under expensive expert
39 supervision.

BACKGROUND TO THE METHOD

40
41 While eye to hand co-ordination and reaction is relatively slow and subject to variability
42 and improvement from practice and eye to voice reaction time is even slower, the
43 reaction time of the eye itself to stimulus is extremely fast in humans and primates. The
44 eye muscles reflexively react to stimuli without the need for conscious action by the
45 subject. Although this reflex can be consciously overridden, the nature of the stimulus
46 and prior fixation can be engineered by methods disclosed in this invention to ensure

1 that the reliability exceeds 97 percent. Furthermore, because the eye reflex is inherently
2 faster than eye-hand or eye-voice reaction times, any variability in the response has a far
3 lower impact on the accuracy of a reaction dependent measurement. This allows the
4 apparatus to exploit the time information in a variety of ways to increase the data
5 obtainable from each individual test point.
6 The invention consists of an eye position-measuring device capable of measurement of
7 eye position at intervals of less than 45 mS of which several types are commercially
8 available in conjunction with a display unit capable of displaying a multiplicity of visual
9 stimuli and capable of accurate calibration of luminance sufficient to exceed the desired
10 accuracy of the desired test. The device is configured to detect the rapid motion of the
11 eye (known as a saccade) towards a new stimulus and to use this saccade to determine
12 the moment the subjects visual reflex responds to the stimulus. Since the subject need
13 not consciously respond to the stimuli the entire field of view measurement process can
14 be automated. By way of example, a set of stimuli can be presented, each stimulus
15 initially below expected threshold increasing in brightness until the stimulus triggers the
16 reflex saccade of the eye from a fixation stimulus. The time the reflex saccade is
17 detected is used to determine the threshold of the retina for that point. The eye
18 position-measuring device can in a preferred embodiment be used to check that the
19 eye's saccade did in fact occur in the correct direction confirming that the test stimulus
20 and not another distraction caused the saccade. At the moment of the said saccade the
21 stimulus that was the saccade target transforms into the fixation point for the next
22 stimulus. This is an important feature for two reasons. First, the accuracy of immediate
23 post saccade fixation has been shown to be consistently many times better than long
24 term fixation on a single point and secondly the visual process of saccading from one
25 stimulus to another in sequence is the normal visual scanning mode of the human and
26 higher primate eye, hence the experience for the patient feels natural and un forced
27 especially if the frequency of the induced saccade is designed to be equivalent to the
28 normal scanning saccade frequency of the eye. This normal scanning frequency varies
29 from time to time in a given individual and from individual to individual but the
30 invention also discloses a method that allows the practitioner to quickly determine this
31 value accurately. Setting the saccade frequency perfectly is not generally necessary but
32 will help to make the test more accurate particularly with anxious patients.
33
34 A major advantage of this method of field of view measurement over the prior art is
35 that it eliminates the need for very large samples to be gathered for each stimuli position
36 and repetitive confirmation of the subject's observation of the stimulus and the
37 reliability of their visual fixation. This vastly reduces the time needed for a diagnostician
38 to establish a subject's field of view.
39 This invention defines a novel method and apparatus which uniquely exploits a detailed
40 computer model of the human visual system's autonomic reflex timings and uses a
41 response interpolator based on this model to allow more accurate interpretation and
42 extrapolation from data while ensuring that the conditions of the test more closely
43 approximate normal visual tasks. This improves both the comfort of the subject and
44 accuracy of the test results. The invention is thus sufficiently accurate to determine
45 progression from one test to another of a fraction of a percent, takes little clinical time
46 to administer and the apparatus itself is economic and easily affordable.
47 In addition to the above benefits the nature of the disclosed method and apparatus also
48 has utility in diagnosis of other visual disorders not directly related to visual field but still
49 dependent on the exploitation of the computer reflex model. This allows the invention
50 to be applied to the diagnosis of high function visual disorders such as dyslexia and
51 visual "neglect". Dyslexia is a higher brain function disorder, which can be improved by
52 appropriate training, and "neglect" is a symptom of a particular form of brain damage.
53

The invention comprises essentially 1. a means to present images to the eye where the luminance of any point in the image over the desired field of view under test can be defined at least as accurately as the desired amplitude accuracy of the retinal map. This display must be capable of presenting an animated fixation image consisting of a substantially stationary central region comprising at least 20 percent of the diameter of the fixation image and a mobile perimeter defined such that the perimeter is less than 3 degrees of the arc of vision of the test subject in diameter. By way of example such a fixation image might consist of an insect such as a ladybird with wiggling legs acting as the mobime perimeter or in a more abstract form a central disk with an eccentric ring with the perigee rotating about the central disk.

2. Means to time the sequence of eye movements and fixations and to determine at least the magnitude but not necessarily the direction of saccades.

3.

4 Means, preferably software means, to present various stimuli to the eye and to instantly replace the stimulus image with the fixation image when triggered by a saccade from the previous fixation image to the stimulus.

5. Means to determine in at least the z-axis the location of the patient's head relative to the screen without constraining the head motion. Suitable means include ultrasonic ranging, laser ranging, stereo or mono video perspective analysis. Various suitable non-contact measurement means are available commercially.

6 A library of images where the sequence and timing of fixations of the typical human eye on the various parts of the image are recorded in a database and means to compare the timing magnitude and sequence of fixations of a test subject to the said database.

Detailed description of the invention

Prior to this invention visual field analysis method and apparatus have been extremely crude, in general consisting of an array of lights or other display illuminated under a pseudo random protocol and at varying brightness straddling the expected threshold of the retina and a fixation point to attempt to maintain some minimal knowledge of the eyes position prior to stimulus. Unfortunately the human vision system is particularly poor at maintaining a constant fixation and furthermore even if this is achieved with practice there are side effects to concentration on a fixation point that significantly reduce the accuracy of the measurement. As a consequence most of these machines are, in practice, little better than the intelligent use of a pen waved at the subject by the practitioner. They provide a rough map of defective areas but the positional accuracy of the defect perimeter is grossly compromised by the impossibility of accurate fixation maintenance by the subject and furthermore the nature of a pursuit or fixed fixation task in itself causes large variations in the subjects' apparent peripheral retinal sensitivity. In research applications with volunteer subjects who are practiced in the use of the instrument these instruments do provide useful data but as a routine diagnostic tool they are simply too complex, time consuming and difficult to use for both the practitioner and the patient.

The following references confirm this assertion:

"Selective Peripheral Fading:

Evidence for Inhibitory Effect of Attention on Visual Sensation"

 Lianggang Lou

Department of Psychology

The University of Hong Kong

1   Barbington-Smith B, 1961 "An unexpected effect of attention in peripheral vision"
2   Nature (London) 189 776
3   Duncan J, 1980 "The locus of interference in the perception of simultaneous stimuli"
4   Psychological Review 87 272-300

5   The prior art of which the following small sample is typical, ignore the nature of the
6   human visual system as a whole. In the absence of such a model the measured values for
7   a given point in the field of view will be tend to be grossly inaccurate both spatially
8   (topologically) and in amplitude terms. The results are akin to plotting the chart of a
9   shoreline with an elastic plumb line and a faulty sextant.
10   As stated above the prior art consists primarily of various methods of presenting varying
11   brightness stimuli to the eye from various angles depending on some form of fixed or
12   moving reference fixation point to deliver geometric accuracy or they include some
13   form of eye tracking system which requires a calibration that is itself subject to the same
14   error of fixation as the untracked test. All of the prior art requires significantly abnormal
15   eye behavior from the subject under test over typically tediously long periods. As the
16   above references show such abnormal fixation behavior inherently destroys both the
17   topological and amplitude accuracy of the data being collected to the point where it is
18   accepted in ophthalmic diagnosis that the repeatability of the measurements can not be
19   better than plus minus 5 degrees and plus minus 2.5dB. Given the progress of common
20   glaucoma at 1.8 percent per annum this means in practice that a confirmed diagnosis of
21   glaucoma can take the several years required to establish the nature of progression with
22   such low repeatability instruments.
23

24

25   EXAMPLES OF THE MOST COMMONLY USED PRIOR ART

26   US4561738 - Field tester
27   Humphrey, William E., San Leandro, CA
28   Campbell, Charles, Berkeley, CA
29   US5050983 - Visual testing method and apparatus
30   Johnson, Chris A, Davis, CA
31   Shapiro, Lionel R., Davis, CA
32   US5024519 - Apparatus and method for visual-field
33   testing
34   Howard, Dwight L., Winters, CA
35   Johnson, Chris A., Davis, CA
36
37   The inventors theorized that if a test method could be devised that allowed the patient
38   to behave as naturally as possible it would consequently be true that the patients
39   autonomic responses would more reliably follow normal repeatable curves. The
40   inventors also researched both fixation and stimulus methods that promote relaxed
41   natural reflex saccades. By carefully researching the limit and variability of these normal
42   responses it would be practical to gather information about the eyes sensitivity and
43   visual field from careful timing of the natural saccade responses to stimuli. This could be
44   applied to several visual stimuli ranging from a carefully sequenced repetitive single
45   point stimulus similar to a conventional visual field analysis method to the presentation
46   of specially formatted images or video sequences where the saccade timing variation
47   between a normal and a visually impaired individual could be made readily apparent.
48

3
4   Unlike the prior art the present invention uniquely exploits an accurate model of the
5   autonomic visual reflexes and interrelated aspects of visual perception in humans and
6   higher primates to vastly improve the accuracy and repeatability of the measurement.
7   This model is incorporated in the timing versus illumination increments described in the
8   method. Additionally the natural interaction of the device with the subject eliminates
9   stress and fatigue in the test that further enhances the repeatability. Uniquely after rapid
10   basic mapping of the visual field the device allows the detailed plotting of any portion of
11   the retina such as the perimeter of a defect to a repeatable accuracy of a fraction of a
12   degree, allowing defect progression rates of 1 degree per annum or less to be detected
13   and characterized by tests separated by weeks rather than years.
14
15
16
17   The models of the autonomic visual reflexes and interrelated aspects of visual
18   perception incorporated in the method and apparatus include the property of the
19   human optical system that perceives stimuli of higher intensity earlier than stimuli of
20   lower intensity. This effect is primarily the consequence of the integrating nature of the
21   retina. The longer a given brightness shines on a given area of the retina the more
22   photons are delivered to the integration until eventually the threshold is crossed, the
23   speed of transit of visual stimuli through the nerve and visual cortex to the brain is also
24   varied by the relative intensity.   This gives rise to the phenomenon known, as the
25   "Pullfrich effect" after the discoverer who described several optical illusions for which
26   the said intensity dependent delay is responsible. It has been used as a method for
27   pseudo stereo image presentation. In the prior art stimuli for visual field analysis have
28   been generally presented for a given fixed time as well as a given brightness so that the
29   threshold of the retina could be determined. This required the sequential and separate
30   presentation of stimuli of different brightness for any given point to establish the
31   threshold of the retina as in US5024519 and others. Such a method is extremely time
32   consuming but hitherto the integration effect precluded the possibility of simply
33   delivering a stimulus of increasing brightness at a given point as there was no way to
34   determine the precise moment that the stimulus was perceived.
35
36   Conversely in the present invention the eyes saccade reflex is modeled in the computer
37   timing so that the moment of perception can be derived from the time interval between
38   the induced saccades. The integration time is exploited to refine the accuracy of the
39   sensitivity measurement of the retina and simultaneously minimize the duration of the
40   test. The equations below demonstrate how this is achieved despite the fact that while
41   the retinal integration is exponential up to the retinal threshold the Pullfrich delay
42   continues to reduce linearly as the stimulus becomes brighter. Hence the time from
43   presentation to the triggering of a saccade will be tens of milliseconds longer for a
44   dimmer stimulus even if both stimuli integrate above the retinal threshold in less than a
45   millisecond. Conversely if the stimuli took 200 mS or more to integrate above threshold
46   the latency delay before the saccade after the retinal threshold is crossed would be much
47   longer than for the previous example so the resulting total delay would be much longer
48   effectively amplifying the time difference between saccades stimulated by different
49   threshold levels of different points on the retina.
50   In conventional static auto perimetry stimuli are presented for a fixed time and so
51   deliver a fixed energy to the retina. The patient is asked to press a button or vocalize if
52   they see a given stimulus at a given point while fixating on a central fixation point.
53   Crucially they must suppress any reflex saccade as best they can to any stimulus during

1. the test. This suppression is uncomfortable to achieve and also causes a subconscious
2. distraction that reduces the patient's accuracy on an already difficult task. Most auto
3. perimeters offer two basic types of test. In one type the stimuli are presented at levels
4. which are just below or just above the expected threshold at a given point and the test is
5. repeated for each point in a "staircase" where if the previous stimulus for a given point
6. caused a patient response then the next stimulus would be presented at 2 to 3 times the
7. desired amplitude resolution below the previous stimulus, and so on till the stimulus
8. fails to generate a patient response. Then a further stimulus is presented halfway
9. between the brightness of the last stimulus that caused a response and the stimulus that
10. failed to cause a response. The final threshold value is then set depending on whether or
11. not the patient responds to this stimulus. Obviously if the patent had failed to respond
12. to the first stimulus in the sequence the next stimulus would be brighter rather than
13. dimmer and the overall sequence would be the reverse of the above. Clearly this method
14. takes a long time, as each point in the retina will typically need five stimuli to determine
15. the threshold. Most auto-perimeters offer an alternative so called "supra threshold" test
16. where each point in the retina is presented at an amplitude calculated on the basis of
17. demographic ophthalmic data to be just above the expected threshold for each point
18. thus a basic plot of areas below a chosen threshold can be plotted. This method is
19. relatively crude of course and does not provide any detailed contour data of the
20. threshold sensitivity.
21. As will be obvious from the above the stimuli are inherently presented in the above tests
22. at or close to the patient threshold. Since the total energy of the stimulus is critical this
23. means that the stimuli are either very dim or of very short duration. In both cases the
24. patient is required to respond consciously to stimuli that in practice are extremely
25. ambiguous. The patient will constantly be marginally aware of stimuli and be
26. consistently uncertain as to whether or not they "saw" a stimulus. Patients report that
27. this is extremely stressful. Practice improves the patient's confidence and so the
28. reliability of the test but such practice is not practical for a routine diagnostic test. The
29. test is further compromised because it is inherently difficult to fixate on a single point
30. accurately. This has two consequences. Clearly if the fixation point is uncertain, then the
31. positional accuracy of any test point on the retina is equally uncertain but the problem is
32. made worse by the fact that the eyes small movements around the fixation mean that
33. the total time a given stimulus illuminates a given point on the retina is variable and so
34. the total integrated energy on that point varies far more than is desirable. The above
35. issues are described to clarify the nature of the present invention.
36. In the present invention the threshold of the retina is determined by the delay between
37. the presentation of a stimulus and the triggering of a reflex saccade to that stimulus. If
38. the stimuli are of low brightness then this time delay will include a period of integration
39. to the point where sufficient energy has been delivered to the retina to pass the
40. threshold and a further delay caused by the Pullfrich effect which makes a brighter
41. stimulus travel faster through the nerve path than a dimmer stimulus. If the stimuli are
42. of higher brightness then the integration time will be shorter and the Pullfrich delay will
43. also be shorter because once the retinal threshold is passed the energy is still integrating
44. on the retina and so the brighter stimulus will travel through the nerve path very much
45. faster. This means that varying the brightness of the stimuli will vary the average time of
46. the saccade response and so the resolution of the amplitude measurement is determined
47. by the resolution of the measured time increment and the chosen brightness. In
48. principle it would be assumed therefore that a dimmer stimuli set would provide a more
49. accurate measure of the retinal amplitude sensitivity as a function of time. While this is
50. true to an extent, the present invention aims to achieve a more accurate spatial plot as
51. well as a more accurate amplitude plot. It is central to this invention that the accuracy of
52. the eye fixation is superior for a few hundred milliseconds post saccade to its accuracy
53. over a longer time therefore the time resolution of the measurement must be balanced

saccades per second the test will feel even more comfortable and natural for the patient. Thus in simplified terms ignoring the integration loss and limit and the precise function of the Pullfrich delay which will be clarified later the time T between the commencement of a stimulus point and the resulting saccade of the eye to that stimulus is expressed by the function

Eq1 :

$$T = \frac{(t^2 \cdot l + P)}{(t \cdot l)}$$

where t is the total time for the luminance "l" to integrate to the detection threshold of the retina and P is the Pullfrich delay for an arbitrarily chosen luminance "h" where $h = t \cdot l$ t can be derived from the function:

Eq2:

$$\left[\frac{-1}{(2 \cdot l)} \cdot \left(-T \cdot l + \sqrt{T^2 \cdot l^2 - 4 \cdot l \cdot P} \right) \right]$$
$$\left[\frac{-1}{(2 \cdot l)} \cdot \left(-T \cdot l - \sqrt{T^2 \cdot l^2 - 4 \cdot l \cdot P} \right) \right]$$

Naturally the greater of the two solutions is the true result since clearly the arbitrarily chosen luminance is chosen to be greater than "l". Hence for any given level of light used as a stimulus the integration time t to h can be determined from the total time T. This means that relative sensitivity of the retina from one point to another is expressed directly as a function of t and can be derived from the interval time T and the resolution of the measure can be adjusted by increasing "l". The overall speed of the test and the average time between saccades can be adjusted for maximum comfort and accuracy by adjusting l to meet the criterion of average saccade time of between 200 and 800 mS described above.

The resulting value of t can be used directly to plot a relative sensitivity map of the retina. However, often it will be required to translate these relative values to commonly used units of measure of the retinal threshold sensitivity. In that case the functions of the retinal integration and the true function of the Pullfrich delay become important. A useful feature of the invention is that the stimulus can be increased or decreased in brightness from its initial presentation brightness, such an increase or decrease can be used to modify the function of T to t to make the resulting function either more or less linear as desired. Clearly in the absence of this feature the dynamic range of the test would be limited if the time intervals are limited as required to maintain a natural rhythm. Increasing the stimulus brightness during presentation is of particular use in the testing of a subject with known defects since the stimuli can be rapidly increased in brightness once a pre determined threshold is passed thus speeding up the test on a subject who would otherwise register a large number of missed stimuli or take so long for each stimulus that the natural comfort rhythm is broken.

The retinal integration function is quite complex as discussed by T E Cohn of Berkeley in his paper "Integration by the human eye; implications for warning signal design". In the typical embodiment of the invention the retinal integration to threshold can be taken as above which follows the standard Blochs Law which states that the product of intensity of a brief flash of light times the time it is on is a constant at threshold. Beyond Bloch's integrating time, usually taken as 0.1sec, **threshold** declines only modestly as duration increases until, for long durations, **threshold** is a constant. This can be enhanced by a simple two-limbed approximation to this **threshold function which**

3 this two-limbed function. It states that the product of a flash intensity times its duration
4 is equal to the asymptotic threshold value times the sum of the duration plus a visual
5 response time constant described above.
6 In certain embodiments of the invention where longer time intervals are desired it may
7 be considered worthwhile to improve the accuracy of the system by utilizing the more
8 accurate Blondel–Rey law however the error induced by the use of the less accurate
9 Blochs Law at the ideal timing intervals recommended for the method are in practice
10 less than errors due to the reflex variables in the eye and so while the overall error
11 budget can be reduced by the use of the most accurate integration formula the accuracy
12 of the Bloch Law embodiment is still substantially better than that achievable by the
13 staircase method in conventional auto perimetry.
14 The Pullfrich function is essentially linear provided the stimuli are of sufficient
15 brightness to exceed threshold in less than 400 mS so again the best performance of the
16 system will be achieved at or close to the natural saccade rhythm of the eye in scanning
17 mode. This natural rhythm has been determined by the inventors in a study of over 150
18 individuals to approximate to within 20 mS a value defined as the subjects "natural
19 counting rhythm". It is well known that people tend to count much faster than once per
20 second and so various word delays are recommended to lengthen the counting rhythm
21 to approximate a second more accurately when people desire to time an event without a
22 watch. The inventors speculated that the natural rhythm would inherently be
23 proportional to the subjects conscious reaction time. It proved to be that a persons
24 expressed maximum comfort zone in terms of saccade frequency exactly matched the
25 subjects natural counting frequency to within 20 mS. This proved to be true despite a
26 variation of well over a factor of two in different individuals natural counting rhythm
27 and also to a similar variation for a given individual in different states of fatigue or
28 arousal. This fact can be used by a practitioner using the invention to set the ideal
29 brightness of the basic illumination level of the stimulus by asking the patient to count
30 up to ten or count aloud the number of items on a screen presentation. The faster the
31 patient counts the brighter the basic stimulus should be for maximum comfort in the
32 test. Alternatively the practitioner can use the count test to determine the patient's level
33 of anxiety and arousal and may take steps to calm the patient until they demonstrate a
34 slower count rhythm and so allow a slower and therefore higher resolution test.
35
36 It should be clear from the above that the accuracy of the test can be enhanced by
37 repeating the test with different basic illumination levels, since the threshold value for a
38 given point and the integration time should correlate exactly. In general however it
39 would not be necessary to repeat the entire test rather the test points for any anomalous
40 areas can be tested again at a different brightness and the integration time measured for
41 that brightness can be correlated with the original data. If the two values agree then the
42 value is certain if they disagree a further test at either of the two previous brightness
43 levels or alternatively at a third brightness level can be applied. If this third test yields
44 anomalous results then the data should be discarded for that point but in practice this
45 occurs in less than one percent of the test points.
46
47 A modified sequence of test stimuli can be presented to create very high spatial
48 resolution plots of a defect perimeter. This is achieved by presenting a sequence of
49 stimuli in a line crossing the perimeter defect alternating with randomly placed stimuli
50 elsewhere to prevent the patient recognizing the pattern. In a preferred embodiment at
51 least some of the alternate stimuli are placed to plot a line to cross other suspected
52 defect perimeter zones. In this later case there should be at least four plot zones
53 randomly sequenced or if less than three suspect zones exist then one or more random

perimeter since the spatial pattern of the plot points would be immediately apparent to the patient. Conversely in the present invention each stimulus that generated a saccade becomes the new fixation point. Combined with the alternating random or alternate zone stimuli this makes the overall spatial pattern perceived by the subject entirely random and unpredictable because although the stimuli are indeed occurring repeatedly on similar points on the retina the overall spatial position of the stimuli as perceived by the subject is not repeating.

In recent years an alternative to basic static automated perimetry has been the frequency-doubling test

One example of this method uses a stimulus that consists of light and dark bars of a low spatial frequency (0.25 cycle/degree), flickering in counter phase at a high temporal frequency (25 Hz). Briefly, the flickering produces an illusion of doubling the spatial frequency of the stimulus. The contrast of the stimulus is gradually increased and the examined subject has to indicate when a movement is perceived anywhere in the visual field. The method is assumed to measure the integrity of a particular subgroup of retinal ganglion cell, sensitive to motion. This type of stimulus can be used with the disclosed saccade trigger in a sequence as described for the point stimulus above where the stimulus changes to the fixation point with each saccade. In this case again the absolute threshold function for the contrast of the bars will correlate to the time T as above hence the range of contrast needed for each presentation of the frequency doubling stimulus target can be reduced because the stimulus need not initially be presented below the contrast threshold since the time for the saccade to the stimulus will indicate the relative level above threshold of the contrast.

In a further embodiment of the invention the relationship between the comfort frequency of the scanning saccade and the normal human visual search saccade frequency can be used to determine if an individual has defects in the retina by presenting each eye individually with pictures based on principles laid out in detail below. These pictures can be natural images or computer generated images with selected regions of high and low spatial frequency in addition to certain visual cues that the inventors have defined which allow the priority of a typical initial search saccade sequence to be reliably predicted. Because in these special images the initial gaze direction of the eye can be predicted with a high reliability and also at least the first saccade from that initial gaze fixation can also be predicted it means that in viewing these images the presence of a high spatial frequency feature on the image will cause the eye to be attracted to it after the initial high priority cue subsequent to the primary gaze fixation. In the normal eye only the blind spot exists as an area that obscures a feature that is revealed to the eye when this initial saccade occurs. If an area of high spatial frequency is revealed as the blind spot moves this causes a change in both the saccade priority AND causes the natural scanning rhythm to "reset" to initial search mode. Since the initial search saccade frequency is much more rapid than the natural scanning frequency any region of high spatial frequency or other high priority cue revealed as the eye initially saccades causing a defect to cease to obscure the said cue will cause a second burst of high frequency saccades as the eye attempts to accommodate for its lack of expected peripheral vision definition by scanning the revealed cues with the fovea. This is an especially useful test since it detects even quite shallow anomalies in the eye even if the contrast differential of the image is much higher than the anomaly depth. The images are designed to cause scanning saccades of relatively small amplitude but the presence of an anomaly will cause a large amplitude saccade as the fovea moves to

accommodate as described above hence both the frequency of the saccades and the amplitude can be used to signal the presence of an anomaly. In this case time from the initial saccade to the triggered saccade is inversely proportional to the depth of the saccade because the differential between the anomaly and the normal portion of the retina is equivalent in practice to the contrast or differential above threshold described for the previous tests in terms of the relationship between stimulus and the speed of the saccade reflex. The location of the saccade spatial frequency cues can be set in a sequence of images to digitally sequence the areas of interest on the retina. For example eight images presented in sequence can detect the presence of an anomaly one 64^{th} of the visual field for each eighth of the visual field tested in each image. Theoretically this could be further refined by further subdivision but in practice it is probably better to revert to either frequency doubling or constant stimulus plotting if detailed plotting is desired. This image test is best used as an "instant" detector of the presence or absence of anomalies worthy of more detailed diagnosis.

Depending on the desire of the practitioner the image colours can be chosen to cover either the full spectrum or selected colours such as blue and yellow that preferentially shows cone anomalies and is therefore more sensitive to relatively small pathologies of the eye.

The basic rules of the image design for predicted priority sequence are as follows:

A solid perspective cue such as road, path or river with a dark end point will draw the first gaze fixation. This will be followed immediately by a saccade to the darkest area of the image coupled with any high spatial frequency data followed by a saccade to the next highest spatial frequency region that is also dark or to the highest spatial frequency area of any brightness if there are no more apparently dark areas of the image. These cues should be set at least ten degrees apart. In a normal vision subject these initial three saccades will occur in less than 400 mS followed by much slower "count" frequency saccades of less than 10 degrees amplitude as the eye assumes normal scanning mode. If however any area of the eye has a defect that uncovers an area of high spatial frequency then the image effectively re triggers the eye brain system to repeat the initial search sequence and so the high frequency high amplitude saccades will continue for at least twice the duration of a normal vision subject.
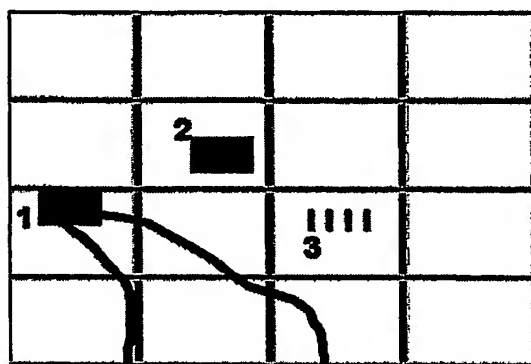
As an example to clarify the principles of the images here are representative figures. Note that the real images may be computer generated photo realistic images or abstract images. The critical aspect is that they follow the principles laid out here.

1
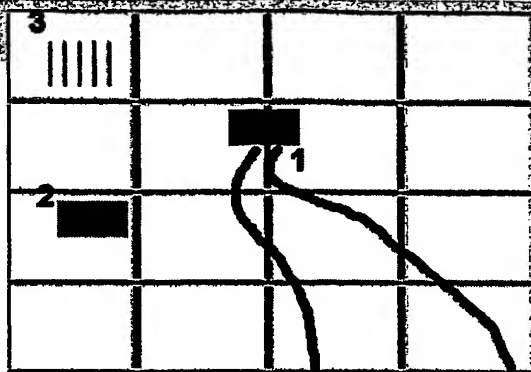
2

3   In the above images the first fixation is marked as 1 the dark area at the end of the
4   "perspective suggesting" path. The area of the retina effectively under test is 3 and the
5   second fixation attractor is 2. In a normal vision subject the spatial frequency attractor at
6   3 does not change during the saccade from 1 to 2 and so does not cause an immediate
7   saccade whereas if a defective area of the retina obscured the high spatial frequency
8   attractor at 3 when fixating on 1 then it would "appear" to the eye immediately after the
9   saccade to 2 and so trigger a reflex saccade. It should be noted that should the subject in
10 fact saccade instead to 3 instead of 2 after 1 this obviously by definition demonstrates
11 that 3 was not under a region of low sensitivity or resolution. This means that this type
12 of test is uniquely free from false positive results which is a great advatage in any
13 screening diagnostic test.

14 . A sequence of images covering the entire field sector by sector can be presented to the
15 patient. The high spatial frequency sector should be no greater than 0.25 degrees per
16 cycle for the areas outside the central ten degrees from the fovea. Ideally the high spatial
17 frequency sector should be more than twice the average spatial frequency of the rest of
18 the image and regions less than half the average spatial frequency should be avoided, as
19 this can tend to alter the saccade priority from the ideal.

20 It should be noted that although the term "perspective" is used this is not intended to
21 mean necessarily true perspective image. The human vision system is so tuned to seek
22 perspective cues that any apparent taper however distorted will tend to be read as a
23 perspective cue. This has been shown in our research to be almost always the primary
24 cue in an image since the brain seeks a sense of scale in any image with an extremely
25 high priority. However areas that suggest shadows or doorways that may obscure
26 potential threats are very high priority too. This proved to be so even with very young
27 subjects the inventors suspect this is a fundamental survival trait that is as genetically
28 programmed as the blink reflex is to an apparent direct threat to the eye. The

3 ever failed to fixate first on such a cue. Note that since the eye saccades to that first cue
4 from its previous rest position no feature of the image is processed by the brain until
5 after the primary gaze fixation.

6 There are many other cues that the inventors have researched that can be arranged in
7 suitable priority sequences to lend further variety to the test but the above listed are
8 adequate to create a successful visual field defect diagnostic tool as disclosed in this
9 patent.

10

11 It should be obvious that instead of a sequence of still images a moving image of many
12 frames per second could be used provided the said moving image could be divided into
13 two or three second sequences where the saccade priorities of each such sequence were
14 known as above. In such a moving image method stimuli that may cause the eye to enter
15 pursuit mode should be avoided.

16 In an alternative method a moving image sequence can be used which is designed to
17 exploit the pursuit mode. In that case the pursuit stimulus should be considered the
18 primary fixation. Wherever the pursuit stimulus comes to rest on the screen can be
19 considered as the primary gaze fixation with the second and third priority cues as
20 defined for the still images above. In this case the timing period used to discriminate
21 normal from abnormal eye behavior should be 2 to 3 second sequences free of the said
22 pursuit stimuli.

23

24 The apparatus may also be used to test for dyslexia using the Fischer method of
25 determining whether and how well the patient is capable of reverse saccades where the
26 patient is instructed to saccade in a direction OPPOSITE to the stimulus. In this
27 invention the method of the test is a presentation of an image of for example the
28 surface of a rabbit warren. The patient is told that a dot will appear just before a rabbit
29 appears exactly opposite from a moving fixation point and they must identify the rabbit
30 from a group of three recognizable "bunnies". The fixation point is for example a bird
31 or fox image moving across the screen at any angle. A red or other colour bright dot
32 appears at some point and within 50mS a rabbit appears for 100 to 150 mS exactly
33 opposite to the dot as measured through the fixation stimulus. Normal subjects will in
34 the majority of cases register one saccade whereas dyslexics will in general register two,
35 one for an aborted saccade to the initial stimulus they are told NOT to look at and one
36 for the correction to the rabbit. This is because the ability of the cognitive system to
37 override the reflex to saccade to any stimulus has proven to be a consistent with the
38 absence of dyslexia whereas the inability to override has proved to be an indication of
39 the opposite. In this invention the proposed "recognition of the rabbit task" or similar
40 recognition task is a strong incentive to saccade as early as possible to see the "rabbit"
41 long enough to recognize it. It is critical to the invention that the features of the rabbit
42 or other recognition task that differentiate it from the other samples previously shown
43 with it to the subject must be of such fine detail as to only be visible to the fovea. If the
44 person waits till the "rabbit" appears before saccading then the saccade will arrive too
45 late for the brain to have time to image the rabbit adequately for recognition. Hence
46 simply suppressing the reflex response to the red dot stimulus is not a solution to the
47 task. Only if the subject saccades opposite to the stimulus will the subject be looking at
48 the point where the rabbit appears and so get enough time with the rabbit imaging on

the fovea to allow recognition. This requires that the eye is capable of saccading at near reflex speed in the opposite direction to the stimulus. This task is possible at about 75 to 90 percent of the time for a normal individual above the age of five. It is impossible for children aged three or less and it is virtually impossible for even mild dyslexics. For example the set of rabbits in the test might be drawn with one two or three sets of whiskers with an apparent diameter of 0.1 to 0.3 degrees. In such a case only the fovea would have sufficient resolution to perceive the whiskers well enough to count them.

The scope of the invention in its broadest aspects is defined in the appended claims. The statements in Appendix I are intended to point out particulalry preferred features and advantages of teh present invention.

1   Apparatus and method comprising at least 1. Means to present images to the eye where the luminance of any point in the image over the desired field of view under test can be defined at least as accurately as the desired amplitude accuracy of the desired test. This display must be capable of presenting an animated fixation image consisting of a substancially stationary central region comprising at least 20 percent of the diameter of the fixation image and a mobile perimeter defined such that the perimeter is less than 3 degrees of the arc of vision of the test subject in diameter.

2. Means to time the sequence of eye movements and fixations and to determine at least the magnitude but not necessarily the direction of saccades.

3.

4 Means, preferably software means, to present various simple stimuli to the eye and to instantly replace the simple stimulus image with the fixation image comprising at least 20 percent of the diameter of the fixation image and a mobile perimeter defined such that the perimeter is less than 3 degrees of the arc of vision of the test subject in diameter, at an instant triggered by a saccade from the previous fixation image to the stimulus.

5. Means to determine in at least the z-axis the location of the patient's head relative to the screen without constraining the head motion. Suitable means include ultrasonic ranging, laser ranging, stereo or mono video perspective analysis. Various suitable non-contact measurement means are available commercially. Contact means which are do not constrain head movement unduly may also be used but are not preferred.

6 A library of images where the sequence and timing of fixations of the typical human eye on the various parts of the image are recorded in a database and means to compare the timing magnitude and sequence of fixations of a test subject to the said database.

2) Means, preferably a software algorithm to calculate the time T between the commencement of a stimulus point and the resulting saccade of the eye to said stimulus expressed by the function

Eq1:

$$T = \frac{(t^2 \cdot 1 + P)}{(t \cdot 1)}$$

Where t is the total time for the luminance "l" to integrate to the detection threshold of the retina and P is the Pullfrich delay for an arbitrarily chosen luminance "h" where

$h = t \cdot 1$ t can be derived from the function:

Eq2:

$$\left[\begin{array}{c} \frac{-1}{(2 \cdot 1)} \cdot \left(-T \cdot 1 + \sqrt{T^2 \cdot 1^2 - 4 \cdot 1 \cdot P} \right) \\[2ex] \frac{-1}{(2 \cdot 1)} \cdot \left(-T \cdot 1 - \sqrt{T^2 \cdot 1^2 - 4 \cdot 1 \cdot P} \right) \end{array} \right]$$

The software algorithm should solve the above equation and use the greater of the two results as the total amplified value sensitivity of a given retinal point stimulated by the apparatus of claim 1 since for any given level of light used as a stimulus the integration

14

3   be derived by the software from the interval time T.

4

5   3) Apparatus as in 1) and 2) where means to vary the resolution of the measurement is
6   provided by adjusting the intensity of "I". The overall speed of the test and the average
7   time between saccades consequently can be adjusted for maximum comfort and
8   accuracy by adjusting "I" to meet the criterion of average saccade time of between 200
9   and 800 mS.

10

11   4) Apparatus as in 1) to 3) where the resulting value of t can be used directly to plot a
12   relative sensitivity map of the retina.

13

14   5) Apparatus as in 1) to 3) where a software algorithm is provided to translate the
15   relative values of T to commonly used units of measure of the retinal threshold
16   sensitivity by look up table or direct function based on the Blondel-Rey law or Bloch
17   law.

18

19   6) Apparatus as in 1) to 5) where the stimulus can be increased or decreased in
20   brightness from its initial presentation brightness during presentation, such an increase
21   or decrease used to modify the function of T to t of claim 2 to make the resulting
22   function either more or less linear. Such means consequently providing means to
23   maintain the overall test speed at a rate most comfortable to the patient.

24

25   7) Apparatus as in 1) where means are provided to simultaneously present several
26   images of a resolution of less than 0.3 degrees only resolvable by the fovea such that the
27   eye is induced to sequentially saccade at the natural saccade frequency of the patients
28   visual scanning mode. Consequently providing a value for this frequency to the
29   computer in the apparatus of claim 1 from which the value of "I" as in claim 2 can be
30   selected to induce a saccade frequency close to the said natural scanning mode.

31

32

33

34   8) Apparatus as in 1) where a sequence of visual stimuli presented on said
35   display in a random or pseudo random sequence such that the position and
36   preferably the expected time of appearance of the next stimulus in a sequence is
37   not readily apparent to a person viewing the display. A device as in the above
38   claims where the timing information is compared to a database of timings for a
39   population of humans of various ages such that the integrated timings of T can
40   be compared to an average population of the same age as the patient under test
41   such that the said value of T can be assigned the value of zero. A further model
42   of the relative normal values of integral T over the full area of the retina such
43   that the normal variations of the retinal sensitivity with respect to angle from
44   fovea may be corrected to zero such that any deviation from the norm will be
45   represented as positive or negative values relative to the normal value.

46   9) A device as in 1) incorporating a database categorized for factors including
47   age that affect the normal sensitivity of the retina and a second database of
48   diseased and other abnormal retinal data that may be compared to the measured
49   retinal data with a view to allowing a software algorithm to suggest a possible
50   diagnosis based on said similarity by means of superposition of perimeter and

sensitivity data for each defect on images of perimeters stored in the database of diseased and other abnormal retinal data. Geometric similarity to a set of images where the set contains a majority of data from a given disease or other abnormal category would trigger the algorithm to suggest the majority disease as the probable diagnosis. Such majorities passed to a second database on confirmation of the said diagnosis over time. This second database is a refined rapid search evolved version of the first database that may be used preferably to the first when it exceeds a sample size of at least 4 times the average majority sample size.

10) A device as in 1) where the display is supplied with images containing a known priority sequence of predictable fixation points at separations of greater than 10 degrees as shown in fig 1 and 2 of approximately half or less the average brightness of the image and where at least one region contains a further sub image of a recognizable structure or alphanumeric character or pictorial representation of an object with a resolution of approximately 0.25 degrees per cycle. Such an image may be for example a cartoon character for a child or an animal picture, while for an adult for example an animal or a vehicle or personality. Means as in claim 1 to time saccade sequences and to deliver an alarm or notification at when more than one sequence of saccades of sub 100mS and greater than 10 degrees occurs per overall image and records the overall time of the sequence of sub 100mS saccades.

11) A device as in 10) where the threshold of 100mS may be varied to accommodate intoxicated brain damaged or other abnormal patients based on an average timing of a sequence of single region of interest images as the norm for a given intoxication, brain impairment or other abnormality.

12) A device as in 9) and 10) where the images are part of a video or moving film sequence

13) A device as in 12) where the primary fixation cue based on fig1 and 2 is replaced with the termination of motion of an image that induces the eye pursuit of said image.

13) A device as in 1) where the image contains a moving stimulus traveling across the display and where a sub image of high detail only capable of discrimination by the fovea may be presented for a period adjustable between 100-600mS within 50 mS of the presentation of a simple bright stimulus on the opposite point of an axis drawn through the moving stimulus. The period of 50mS is a preferred value but any value that is shorter than the time required by the subject to saccade to the simple stimulus and back to the complex stimulus is intended. Faster values might prove to be more reliable with patients trained in sports and so practiced in faster saccades. In other cases slower values may be suitable for patients suffering from brain impairments. Said device used to diagnose dyslexic characteristic inability to saccade opposite to a stimulus.

14) A device as in 1) where means are provided to illuminate the eye preferably in the infra red region capable of creating a clear highlight on the cornea as viewed by the camera and means whereby the camera delivers images in an electronically interpretable way to a calculating device such that the highlight reflections of the cornea of both motion blurred and non blurred images may be analyzed by commercially

available software algorithms to determine the angular moments of the
blur which in turn defines the direction of the eyes movement causing
the motion blur. Such means used to interpret the saccade results to
confirm that the saccades were induced by the stimulus and not other
distraction

15) A device as in any or all of the above where the essential timing, control and
display mechanisms are embodied in a software package capable of exploiting
commercially available display, camera and measurement devices to fulfill the
objectives.

1 <u>CLAIMS</u>

2

3 1.   A method of assessing eye function, comprising:

4   (a)   presenting images to the eye where the

5 luminance of any point in the image over the desired

6 field of view under test can be defined at least as

7 accurately as the desired accuracy of a retinal map

8 to be obtained;

9   (b)   forming said images to provide an animated

10 fixation image comprising a substantially stationary

11 central region comprising at least 20% of the

12 fixation image and a mobile perimeter defined such

13 that the perimeter is greater than 3% of the arc of

14 vision of the test subject in diameter;

15   (c)   presenting a simple stimulus to the eye;

16   (d)   detecting a saccade triggered by said

17 simple stimulus and immediately replacing the simple

18 stimulus with a fresh animated fixation image;

19   (e)   recording the timing and magnitude of the

20 saccade and the subsequent fixation;

21   (f)   repeating steps (e) to (c); and

22   (g)   comparing the results with a database of

23 typical eye responses.

24

25 2.   The method of claim 1, further including

26 determining the location of the subject's head

27 relative to the image in at least the z-axis,

28 without applying any constraint to the head motion.

29

30 3.   Apparatus for use in assessing eye function,

31 comprising:

1   (a)   display means for presenting images to the

2   eye where the luminance of any point in the image

3   over the desired field of view under test can be

4   defined at least as accurately as the desired

5   accuracy of a retinal map to be obtained;

6   (b)   means for generating on the display means

7   an animated fixation image comprising a

8   substantially stationary central region comprising

9   at least 20% of the fixation image and a mobile

10   perimeter defined such that the perimeter is greater

11   than 3% of the arc of vision of the test subject in

12   diameter;

13   (c)   means for generating a simple stimulus on

14   the display means;

15   (d)   means for detecting a saccade triggered by

16   said simple stimulus and immediately replacing the

17   simple stimulus with a fresh animated fixation

18   image;

19   (e)   means for recording the timing and

20   magnitude of each saccade and subsequent fixation

21   and for comparing the results with a database of

22   typical eye responses.

23

24   4.   Apparatus according to claim 3, further

25   including means for determining the location of the

26   subject's head relative to the image in at least the

27   z-axis, without applying any constraint to the head

28   motion.

29

30

PCT/GB2004/001700

‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖‖